

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau




(43) International Publication Date
9 October 2003 (09.10.2003)

(10) International Publication Number
PCT WO 03/083778 A1

- (51) International Patent Classification⁷: **G06T 11/00**,
A61B 5/055, 6/03
- (21) International Application Number: **PCT/IB03/01122**
- (22) International Filing Date: **24 March 2003 (24.03.2003)**
- (25) Filing Language: **English**
- (26) Publication Language: **English**
- (30) Priority Data:
102 14 254.8 **30 March 2002 (30.03.2002)** **DE**
- (71) Applicant (for DE only): **PHILIPS INTELLECTUAL PROPERTY & STANDARDS GMBH [DE/DE]**; Stein-damm 94, 20099 Hamburg (DE).
- (71) Applicant (for all designated States except DE, US): **KONINKLIJKE PHILIPS ELECTRONICS N.V. [NL/NL]**; Groenewoudseweg 1, NL-5621 BA Eindhoven (NL).
- (72) Inventors; and
(75) Inventors/Applicants (for US only): **KATSCHER, Ul-rich [DE/DE]**; Philips Intellectual Property & Standards GmbH, Weissshausstr. 2, 52066 Aachen (DE). **KÖH-LER, Thomas [DE/DE]**; Philips Intellectual Property & Standards GmbH, Weissshausstr. 2, 52066 Aachen (DE). **SCHMIDT, Thomas [DE/DE]**; Philips Intellectual Prop-erty & Standards GmbH, Weissshausstr. 2, 52066 Aachen (DE).
- (74) Agent: **MEYER, Michael**; Philips Intellectual Property & Standards GmbH, Weissshausstr. 2, 52066 Aachen (DE).
- (81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PH, PL, PT, RO, RU, SC, SD,

[Continued on next page]

(54) Title: **ORGAN-SPECIFIC BACKPROJECTION**

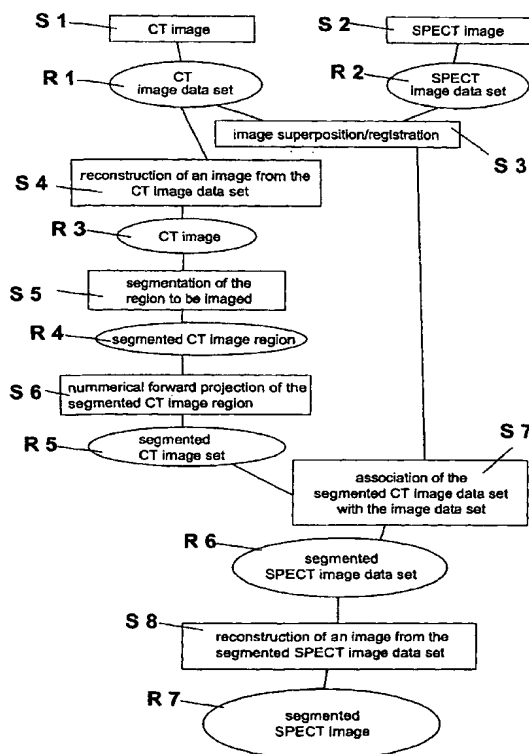

(57) Abstract: The invention relates to a method for the selective imaging of body structures, in which method - a first image data set is acquired by means of a first tomography method, - a second image data set is acquired by means of a second tomography method which has a resolution which is higher than that of the first method, the image data of the first and the second image data set coinciding at least partly in space, - an image is reconstructed from the first image data set, and - the image data to be imaged is selected from the first image data set by means of the second image data set. In order to achieve a higher imaging quality while using a low-resolution tomography method, in accordance with the invention it is proposed that for the image reconstruction from the first image data set - first at least one image region to be imaged is selected from the second image data set, and - subsequently the image reconstruction is calculated from the image data of the first image data set which are situated in the selected image region.



WO 03/083778 A1



SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US,
UZ, VC, VN, YU, ZA, ZM, ZW.

SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM,
GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(84) Designated States (regional): ARIPO patent (GH, GM,
KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),
Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE,
ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO,

Published:

— with international search report

*For two-letter codes and other abbreviations, refer to the "Guid-
ance Notes on Codes and Abbreviations" appearing at the begin-
ning of each regular issue of the PCT Gazette.*

3/PARTS

10/510005

DT04 Rec'd PCT/PTO 30 SEP 2004

WO 03/083778

PCT/IB03/01122

1

Organ-specific backprojection

The invention relates to a method for the selective imaging of body structures, in which method

- a first image data set is acquired by means of a first tomography method,
 - a second image data set is acquired by means of a second tomography
- 5 method which has a resolution which is higher than that of the first method, the image data of the first and the second image data set coinciding at least partly in space,
- an image is reconstructed from the first image data set, and
 - the image data to be imaged is selected by means of the second image data
- set.

10 The invention also relates to a device for the selective imaging of body structures in conformity with the described method and to a computer program which is to be executed on a computer and comprises programming means for executing the described steps of the method.

Many tomography methods, notably tomography methods intended for nuclear
15 medicine, such as SPECT (Single Photon Emission Computed Tomography) or PET (Positron Emission Tomography) methods, have the advantage that they provide the viewer of the tomographically formed image with information which goes beyond pure morphology and that in some cases they also visualize physiological processes. Such tomography methods have the drawback, however, that they have only a low spatial resolution so that often only a
20 very poor imaging quality is achieved, notably for fine structures.

In order to avoid this drawback it is known to combine said tomography method with a further tomography method. The second tomography method then images the same region as the previously described tomography method having the low resolution. On the basis of the second tomography method, having a higher resolution, the viewer can then
25 select a given region of interest from the overall image; very exact selection (so-called segmentation) is then possible because of the high resolution of the second method. Subsequently, that region of the low-resolution tomography image, produced by the first, low-resolution tomography method, which corresponds to the selected region of the high-resolution tomographic image is associated therewith by way of image registration, and

exclusively this region is imaged. A method of this kind is described in the article "Iterative Reconstruction of Emission Tomography Data with A Priori Information", Vollmar St. et al., Transactions on Medical Imaging, 1999.

5 This type of combination of two tomography methods has the drawback that
the original image acquired by means of the low-resolution tomography method is
reconstructed in a conventional manner and that the selection of a detail of this image by
means of the high-resolution method takes place only at a later stage. For the conventional
reconstruction of the image, the acquired image data are backprojected regularly; during such
backprojection the signals measured during the image acquisition by way of forward
0 projection are distributed along the relevant projection line across the entire image region.
Because of this distribution across the entire image region, the signals become unsharp and
the distance-to-noise ratio becomes small. Experts in this field refer to this phenomenon as
"smearing".

Such smearing is particularly disadvantageous when an iterative method is
5 used for the backprojection, because the smearing and the large image region to be measured
necessitate a large number of iterations, thus prolonging the required calculation time and
effort.

Therefore, it is an object of the invention to provide a method which enables a
higher imaging quality to be achieved for a low-resolution tomography method. It is also an
0 object of the invention to provide a device and a computer program for carrying out said
method.

The object is achieved in accordance with the invention in that for the image
reconstruction from the first image data set

5 - first at least one image region to be imaged is selected from the second image
data set, and

- subsequently the image reconstruction is calculated from the image data of
the first image data set which are situated in the selected image region.

Therefore, the method in accordance with the invention does not calculate a
backprojection across the entire image region during the image reconstruction. Instead, an
0 image region which is of interest to the viewer is selected in advance. This selection is
performed on the basis of image data which have been acquired by means of a second
tomography method having a resolution which is higher than that of the first tomography
method. It is notably possible to select regions of the image which contain the object to be

imaged or parts thereof. Furthermore, it is also possible to select a number of regions which may also be coherent, for example, vascular systems.

The backprojection of the image data across the selected image region ensures that the image values are not smeared across the entire image region, but only across a
5 smaller image region, that is, the selected image region. It is thus achieved that the signal-to-noise ratio (SNR) is increased and the quality of the images of the structures to be imaged is enhanced.

The method in accordance with the invention is advantageous notably when the first tomography method is a nuclear-medical tomography method, notably a SPECT
10 method or a PET method. According to such methods, a contrast medium is administered to the patient prior to the tomographic acquisition of the image data. This contrast medium concentrates in given structures of the body, possibly in dependence on given physiological processes, and is imaged with a high contrast by the nuclear medical tomography method. SPECT and PET then have only a low spatial resolution of from approximately 5 to 15 mm.
15 In order to enhance the image quality, use can notably be made of a magnetic resonance tomography method or an X-ray tomography method (MR and CT, respectively). These tomography methods have a resolution in the range of from 0.5 to 1 mm. The use of the method in accordance with the invention is advantageous in particular when a combined CT/PET system or another tomography apparatus combining other tomographic methods is
20 used for the tomographic imaging.

According to an advantageous version of the method the selection of the image region is performed by means of an automatic segmentation method.

In addition to the manual segmentation by the viewer, for example, by defining image boundaries or by selecting image corner points, notably automatic selection
25 methods are advantageously used. According to the automatic selection methods, for example, a selection of the image elements to be imaged can be carried out on the basis of their image values (for example, grey values). For example, it is possible to select given body tissues on the basis of the image values of a computed tomography X-ray image (so-called HU values), said body tissues then being imaged or excluded from imaging. Furthermore, it
30 is feasible for an automatic segmentation method to select regions which have the same or a similar image value and are coherent. Conventional segmentation methods, for example, the so-called regional growing method, can then be used. It may also be arranged that other methods, such as morphological opening or the like, are used for the automatic selection of an image region.

The method in accordance with the invention may ensure in particular that the necessary association of the image data of the first and the second image data set with one another, that is, the so-called registration, is simplified or accelerated by associating exclusively image data of the first image data set which are to be imaged with the second
5 image data set.

It is particularly advantageous to use the method in accordance with the invention when the image reconstruction is carried out by way of iterative backprojection. An iterative calculation then takes place in principle in such a manner that the difference is formed between intermediate results of an image calculation which is periodically performed
0 in the same manner is formed and that the quality of the calculated image is evaluated on the basis of the value of the difference between two successive calculation cycles. Normally speaking, a limit value (convergence criterion) to be reached is then defined.

Because the distance between the signal and the noise value is increased from the very start of the method in accordance with the invention, the method in accordance with
5 the invention enables a reduction of the number of iteration steps required until a convergence criterion is met, that is, in comparison with the conventional method with smearing across the entire image region. Analogously, when the number of iteration steps in the method in accordance with the invention is kept the same as in conventional methods, the image quality of the image formed by means of the method in accordance with the invention
0 can be enhanced in comparison with the image quality of the image reconstructed in a conventional manner.

A further aspect of the invention concerns a device for the selective imaging of body structures, which device includes first tomographic image data acquisition means, second tomographic image data acquisition means, having a resolution which is higher than
5 that of the first tomographic image data acquisition means, means for image reconstruction by backprojection of an image, notably from a first image data set which has been acquired by means of the first tomographic image data acquisition means, and selection means for selecting at least one region of the image data to be imaged, preferably by selection of one or more regions of an image which has been derived from the second image data set. The
0 backprojection means co-operate with the selection means in such a manner that during the backprojection of the image data exclusively the image data are projected which are situated in the selected image region which was selected, by way of the second image data set, by the selection means.

Finally, a last aspect of the invention concerns a computer program with programming means for making a computer carry out the method of claim 1 when the computer program is executed on a computer.

5

A preferred embodiment of the invention will be described in detail hereinafter with reference to the Figures. Therein:

Fig. 1 shows a flow chart of a method in accordance with the invention,

Fig. 2 is a diagrammatic representation of the co-operation of the means of a
10 device in accordance with the invention, and

Fig. 3 shows a flow chart of a method for iterative backprojection.

As is shown in Fig. 1, in conformity with the preferred version of the method
15 in accordance with the invention first a computed tomography image S1 of a body region is formed; for this purpose several slice images of this body region are acquired at a given distance from one another. This computed tomography image yields a CT image data set R1. Before or after the computed tomography image acquisition, a contrast medium is administered to the patient and a SPECT image S2 is formed, resulting in a SPECT image
20 data set R2. The SPECT image S2 is preferably formed for the same body region and while using the same distance between the slice planes as for the CT image S1.

For the CT image data set R1 and the SPECT image data set R2 there is performed an image superposition or registration operation S3 in which the image data of the CT image data set R1 which are situated in the same geometrical position as the image data
25 of the SPECT image data set R2 are associated with one another. Known methods, for example, fiducial markers can be used for such association. The CT image S1 and the SPECT image S2 need not necessarily cover an identical image region, but it suffices when the two images overlap in the region to be imaged. Furthermore, it is not necessary either for the spacing of the slices of the two images to be the same; it is also feasible that the distance
30 between the slices of one image amounts to an integer multiple of the distance between the slices of the other image.

An image S4 is then reconstructed from the CT image data set R1; customary methods, such as iterative or analytic backprojection, can be used for this purpose. In the CT image R3 thus formed a segmentation of the region S5 to be imaged is performed. This

segmentation can take place in a direction orthogonal as well as in a direction parallel to the projection direction, notably simultaneously in both directions. For example, a region to be imaged can be defined by setting a plurality of corner points of a region to be imaged or by drawing a boundary line around a region. It is also possible to select a plurality of regions to be imaged which are connected to one another or not. Furthermore, it is feasible for the segmentation to be executed automatically by the selection of image elements having a given range of image values or by the selection of coherent regions having a similar range of image values, for example, by way of the so-called region growing method. Furthermore, it is feasible to select structures in the image which are smaller or larger than a given value; customary methods, such as the morphological opening method, can be used for this purpose. It is also feasible to remove one or more image regions from the region to be imaged by means of a filtering operation.

The segmented CT image R4 thus formed is converted into a segmented CT image data set R5 by way of a numerical forward projection S6. During this step, the selected image elements, that is, the segmented region to be imaged, can be associated again with the image data of the original CT image data set in a simplified manner.

The image data of the segmented CT image data set are associated with the image data of the SPECT image data set in a next step S7, resulting in a segmented SPECT image data set R6. This segmented SPECT image data set R6 contains only the image data which are of relevance for the region to be imaged as selected on the basis of the CT image data set. In a further step S8 an image is reconstructed from the segmented SPECT image data set, that is, preferably by iterative backprojection of the segmented SPECT image data set. During this iterative backprojection, the image data is smeared only across the region to be imaged, so regularly across a region which is substantially smaller than the overall image region, thus enhancing the signal-to-noise ratio. The image R7 thus reconstructed has sharper edges and contains more contrast. This reduces the number of iteration steps required for an image whose quality is substantially equivalent to that of an image obtained by means of a conventional reconstruction technique, meaning that the required calculation time and effort are less. Analogously, when the number of iteration steps is the same as that of the conventional method, that is, while spending the same calculation time and calculation effort, an image of significantly higher quality can be formed.

Fig. 2 is a diagrammatic representation of the construction of the device in accordance with the invention and of the programming means of the computer program in accordance with the invention.

The device comprises CT image acquisition means M1 and SPECT image acquisition means M2 which co-operate with image superposition or registration means M4. The CT image acquisition means M1 co-operate with image reconstruction means M3 for the CT image, which means form a CT image from the CT image data set. This CT image is segmented by means of manual segmentation means M5 which are controlled by a user of the device, thus selecting a region to be image.

The manual segmentation means co-operate with means for the numerical forward projection M7 of the selected CT image elements which form an image data set from the segmented image.

Alternatively, as is denoted by the dashed lines in Fig. 2, the CT image acquisition means can co-operate with automatic segmentation means M6 which automatically select given data on the basis of preset parameters or parameters which can be influenced by the user of the device.

The image data selected by means of the automatic segmentation means M6 or the image data produced by means of the numerical forward projection means, co-operate with image reconstruction means M8 for the SPECT image data. The image reconstruction means for the SPECT image data co-operate with the image superposition/registration means so as to associate the selected CT image data with the corresponding, geometrically identically situated SPECT image data.

Alternatively it may also be arranged to perform the image superposition or registration by means of the image superposition means M4 only at an instant after a manual (M5) or automatic (M6) segmentation, and hence also selection of the image elements to be imaged, has taken place. In that case there is no superposition of image regions or registration of image data which are not situated in a region to be imaged.

The image reconstruction means SPECT M8 form a high-quality nuclear medical image of the segmented image region from the selected image data.

The reconstruction of an image from the segmented SPECT image data set S8 by way of iterative backprojection will be described with reference to Fig. 3. The iteration consists in that first, in a backprojection S10, an iteration image R11 is calculated by backprojection of the image data to be imaged of the first image data set R6, selected on the basis of the second image data set or the image R1, R3, after which an iteration image data set R12 is numerically formed from this iteration image R11 in a calculation step S11. This iteration image data set R12 thus represents the result of a numerical forward projection S11 of the calculated image. Subsequently, a difference is formed between the numerically

formed iteration image data set R12 and the first image data set R10. This difference is a measure of the deviation between the iteration image data set R12 and the iteration start image data set R10. If this difference is particularly small, the calculated image does not constitute a significant qualitative improvement relative to the initially calculated image. In
5 this case the iterative calculation process is terminated and the calculated image R11, R7 is output via an output S20.

When the difference does not drop below a predetermined value (the convergence criterion), however, the difference is added to the iteration image data set S11 and a new iteration start image data set R14 is calculated. Using this calculated iteration start
0 image data set R14, representing the new iteration start image data set R10, subsequently an iteration operation is started again, at the end of which the difference is again used for evaluating the convergence and, should the convergence criterion not be satisfied, the difference is again added to the iteration image data set R12 so as to form an iteration start image data set R14.

5 The above iteration steps are repeated until the convergence criterion is satisfied and the image R11 last calculated is output to the viewer as a segmented SPECT image R7.

CLAIMS:

1. A method for the selective imaging of body structures, in which method
 - a first image data set is acquired by means of a first tomography method,
 - a second image data set is acquired by means of a second tomography method which has a resolution which is higher than that of the first method, the image data of
- 5 the first and the second image data set coinciding at least partly in space,
 - an image is reconstructed from the first image data set, and
 - the image data to be imaged is selected from the first image data set by means of the second image data set,
- characterized in that for the reconstruction from the first image data set
- 0
 - first at least one image region to be imaged is selected from the second image data set, and
 - subsequently the image reconstruction is calculated from the image data of the first image data set which are situated in the selected image region.
- 5 2. A method as claimed in claim 1, characterized in that the first tomography method is a nuclear medical tomography method, notably SPECT or PET.
3. A method as claimed in claim 1, characterized in that the selection of the image region is performed by means of an automatic segmentation method.
- 0 4. A method as claimed in claim 1, characterized in that the image reconstruction is carried out by way of iterative backprojection.
- 5 5. A method as claimed in claim 4, characterized in that the calculation of the image consists of the initial calculation of an image by backprojection of the image data to be imaged of the first image data set, the following steps
 - numerical formation of an iteration image data set from the calculated image,
 - determination of the difference between the first image data set and the iteration image data set,

- calculation of an iteration image by addition of the difference to the calculated image, and the iterative repetition of these steps for the calculated iteration images until at least one convergence criterion is satisfied, that is, notably the difference dropping below a predetermined convergence value.

5


6. A device for the selective imaging of body structures, which device includes
- first tomographic image data acquisition means for the acquisition of a first image data set,

- second tomographic image data acquisition means for the acquisition of a
.0 second image data set, which second tomographic image data acquisition means have a resolution which is higher than that of the first tomographic image data acquisition means,

- backprojection means for image reconstruction of an image from the first image data set, and

- selection means for selecting, by means of the second image data set, the
.5 image data to be imaged, characterized in that the backprojection means co-operate with the selection means in such a manner that the image is calculated exclusively from the image data of the first image data set which are situated in the selected image region.

7. A computer program which includes programming means for making a
!0 computer carry out the method claimed in claim 1 when the computer program is executed on a computer.

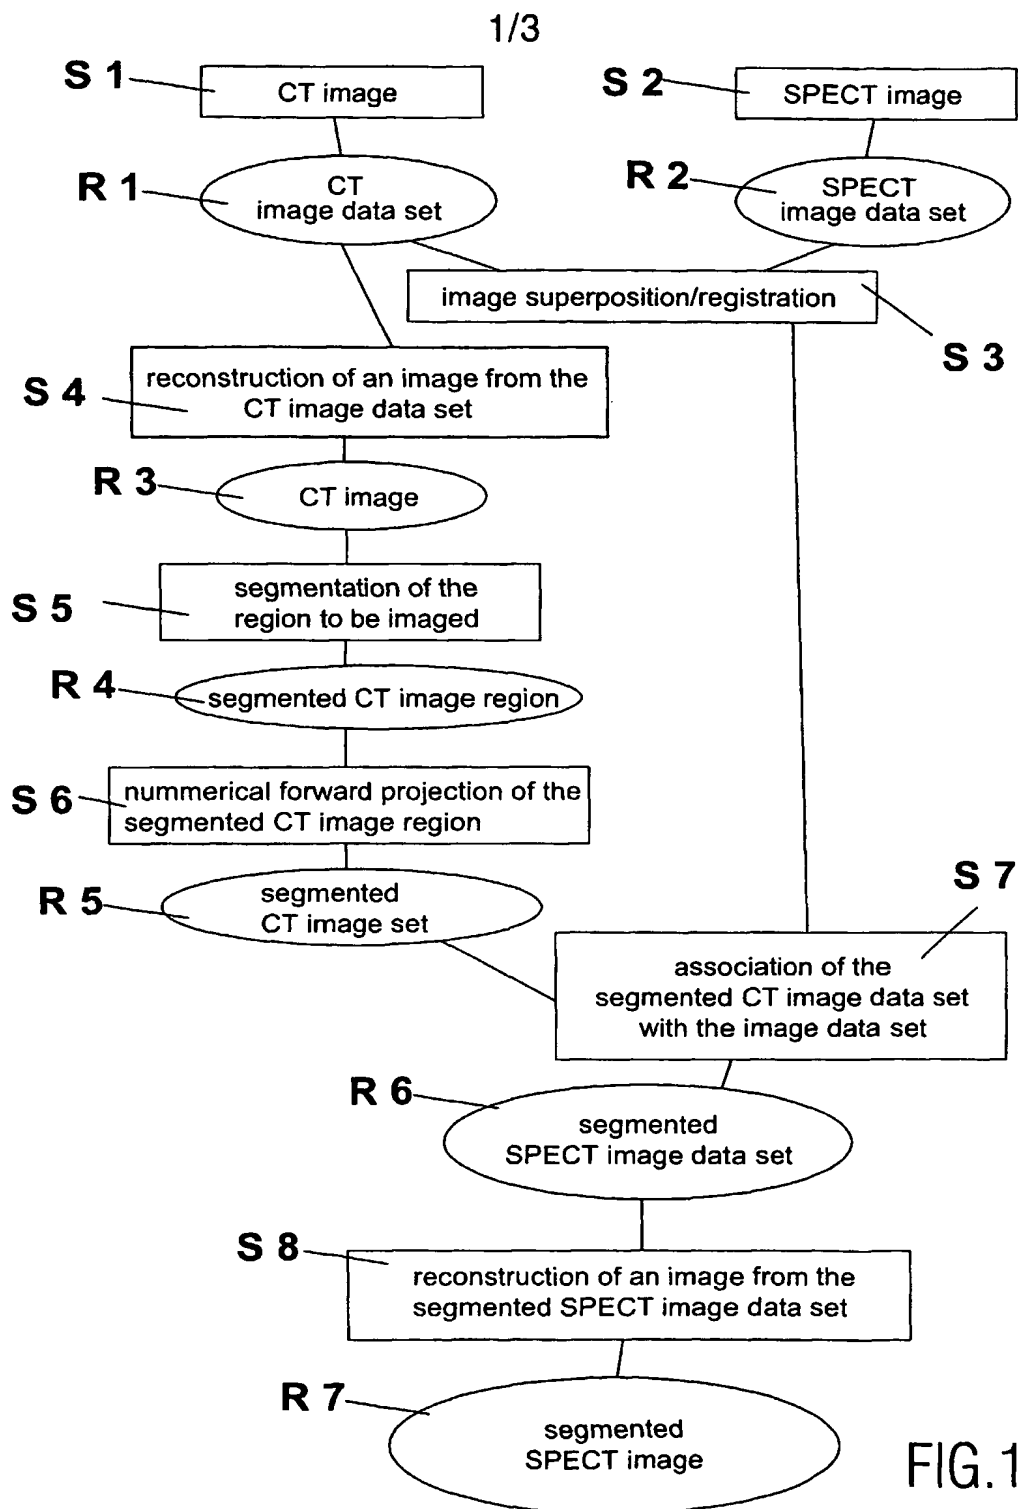

2/3

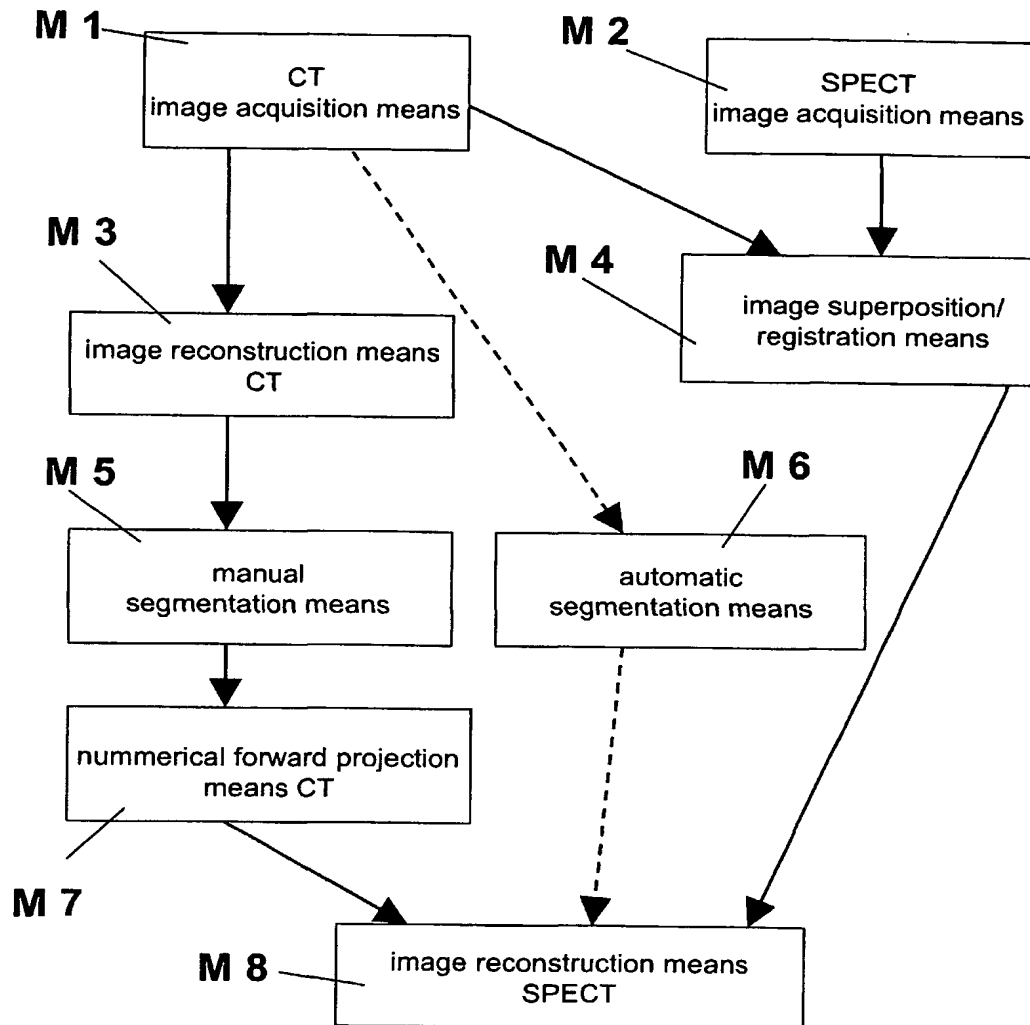


FIG.2

3/3

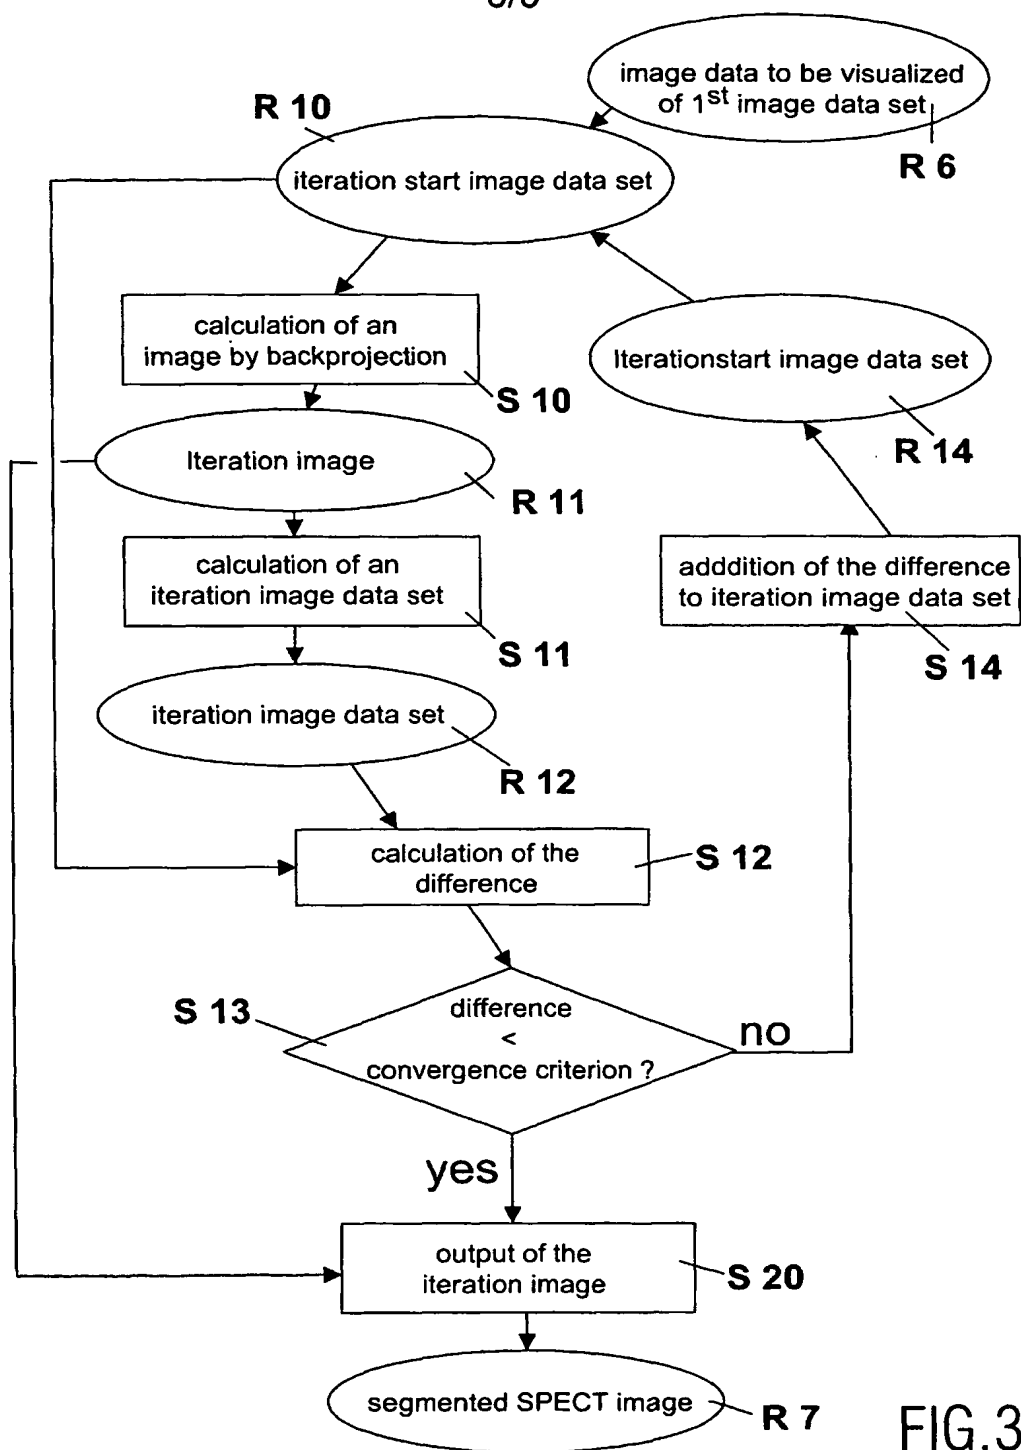


FIG.3

INTERNATIONAL SEARCH REPORT

PCT/IB 03/01122

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 G06T11/00 A61B5/055 A61B6/03

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 G06T A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the International search (name of data base and, where practical, search terms used)

EPO-Internal, INSPEC

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X ✓	LIPINSKI ET AL.: "Expectation Maximization Reconstruction of Positron Emission Tomographic Images Using Anatomical Magnetic Resonance Information" IEEE TRANSACTIONS ON MEDICAL IMAGING, vol. 16, no. 2, 1 April 1997 (1997-04-01), pages 129-136, XP002244909 page 129, left-hand column, paragraph 1 -page 130, left-hand column, paragraph 3 page 134, right-hand column, paragraph 2 -page 136, left-hand column, paragraph 1 abstract --- -/--	1-7

☒ Further documents are listed in the continuation of box C.

☐ Patent family members are listed in annex.

* Special categories of cited documents:

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

& document member of the same patent family

Date of the actual completion of the international search

19 June 2003

Date of mailing of the international search report

02/07/2003

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Manschot, J

INTERNATIONAL SEARCH REPORT

PCI/18 03/01122

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X ✓	<p>YONG ZHANG ET AL: "Incorporating MRI region information into SPECT reconstruction using joint estimation" ACOUSTICS, SPEECH, AND SIGNAL PROCESSING, 1995. ICASSP-95., 1995 INTERNATIONAL CONFERENCE ON DETROIT, MI, USA 9-12 MAY 1995, NEW YORK, NY, USA, IEEE, US, 9 May 1995 (1995-05-09), pages 2307-2310, XP010151802 ISBN: 0-7803-2431-5 page 2307, left-hand column, paragraph 1 -page 2308, right-hand column, paragraph 2.2 abstract</p>	1-7
A ✓	<p>----- VOLLMAR ST ET AL: "Iterative reconstruction of emission tomography data with a-priori-information" NUCLEAR SCIENCE SYMPOSIUM, 1998. CONFERENCE RECORD. 1998 IEEE TORONTO, ONT., CANADA 8-14 NOV. 1998, PISCATAWAY, NJ, USA, IEEE, US, 8 November 1998 (1998-11-08), pages 1560-1561, XP010338179 ISBN: 0-7803-5021-9 cited in the application the whole document -----</p>	1,2,4,6, 7

